



Neutral Invertase Microplate Assay Kit

User Manual

Catalog # ASK1027

Detection and Quantification of Neutral Invertase (NI) Activity in
Tissue extracts, Cell lysate Samples.

For research use only. Not for diagnostic or therapeutic procedures.

Bioworld Technology, Inc. (USA)

Email: info@bioworld.com

Web: www.bioworld.com

Bioworld technology, co. Ltd. (China)

Email: info@biogot.com

Web: www.biogot.com



I. INTRODUCTION.....2

II. KIT COMPONENTS.....3

III. MATERIALS REQUIRED BUT NOT PROVIDED.....3

IV. SAMPLE PREPARATION.....4

V. ASSAY PROCEDURE.....5

VI. CALCULATION.....6

VII. TYPICAL DATA.....7



I. INTRODUCTION

Invertase, also known as sucrase or β -fructofuranosidase, catalyzes the hydrolysis of sucrose by cleaving its glycosidic bond and forming one molecule each of glucose and fructose. According to the optimum pH, invertase is divided into acid invertase (AI) and neutral invertase (NI).

NI mainly exists in the cytoplasm, responsible for the decomposition of sucrose to fructose and glucose in the cytoplasm.

NI hydrolyzes the sucrose to generate reducing sugar. The reducing sugar reduces the 3,5-dinitrosalicylic acid to generate red-brown substance. The color intensity, measured at 540 nm, is proportionate to the enzyme activity in the sample.



II. KIT COMPONENTS

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer	30 ml x 4	4 °C
Reaction Buffer	20 ml x 1	4 °C
Substrate	Powder x 1	4 °C
Dye Reagent	10 ml x 1	4 °C
Standard	Powder x 1	4 °C
Plate Adhesive Strips	3 Strips	
Technical Manual	1 Manual	

Note:

Substrate: add 8 ml Reaction Buffer to dissolve before use.

Standard: add 1 ml distilled water to dissolve before use, the concentration will be 3 mmol/L.

III. MATERIALS REQUIRED BUT NOT PROVIDED

1. Microplate reader to read absorbance at 540 nm
2. Distilled water
3. Pipettor
4. Pipette tips
5. Mortar
6. Ice
7. Centrifuge
8. Timer
9. Convection oven



IV. SAMPLE PREPARATION

1. For tissue samples

Weigh out 0.1 g tissue, homogenize with 1 ml Assay buffer on ice, centrifuged at 12,000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

2. For cell and bacteria samples

Collect cell or bacteria into centrifuge tube, discard the supernatant after centrifugation, add 1 ml Assay buffer for 5×10^6 cell or bacteria, sonicate (with power 20%, sonication 3s, interval 10s, repeat 30 times); centrifuged at 12000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.



V. ASSAY PROCEDURE

Add following reagents into the microcentrifuge tubes:

Reagent	Sample	Control	Standard	Blank
Sample	20 µl	--	--	--
Reaction Buffer	--	20 µl	--	--
Substrate	80 µl	80 µl	--	--
Mix, put it in the oven, 37 °C for 30 minutes. Then put it in boiling water for 10 minutes. Add the supernatant into the microplate.				
Supernatant	100 µl	100 µl	--	--
Standard	--	--	100 µl	--
Distilled water	--	--	--	100 µl
Dye Reagent	100 µl	100 µl	100 µl	100 µl
Mix, put it into the convection oven, 90 °C for 10 minutes, record absorbance measured at 540nm.				

VI. CALCULATION

Unit Definition: One unit of NI activity is the enzyme that generates 1 μmol of reducing sugar per minute.

1. According to the protein concentration of sample

$$\begin{aligned}\text{NI (U/mg)} &= C_{\text{Standard}} \times V_{\text{Standard}} \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (V_{\text{Sample}} \times \\ & C_{\text{Protein}}) / T \\ &= 0.5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / C_{\text{Protein}}\end{aligned}$$

2. According to the weight of sample

$$\begin{aligned}\text{NI (U/g)} &= C_{\text{Standard}} \times V_{\text{Standard}} \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (W \times V_{\text{Sample}} \\ & / V_{\text{Assay}}) / T \\ &= 0.5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / W\end{aligned}$$

3. According to the quantity of cell or bacteria

$$\begin{aligned}\text{NI (U/10}^4\text{)} &= C_{\text{Standard}} \times V_{\text{Standard}} \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (N \times \\ & V_{\text{Sample}} / V_{\text{Assay}}) / T \\ &= 0.5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / N\end{aligned}$$

C_{Standard} : the concentration of Standard, 3 mmol/L = 3 $\mu\text{mol/ml}$;

C_{Protein} : the protein concentration, mg/ml;

W: the weight of sample, g;

V_{Standard} : the volume of standard, 0.1 ml;


V_{Sample} : the volume of sample, 0.02 ml;

V_{Assay} : the volume of Assay buffer, 1 ml;

T: the reaction time, 30 minutes.

VII. TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

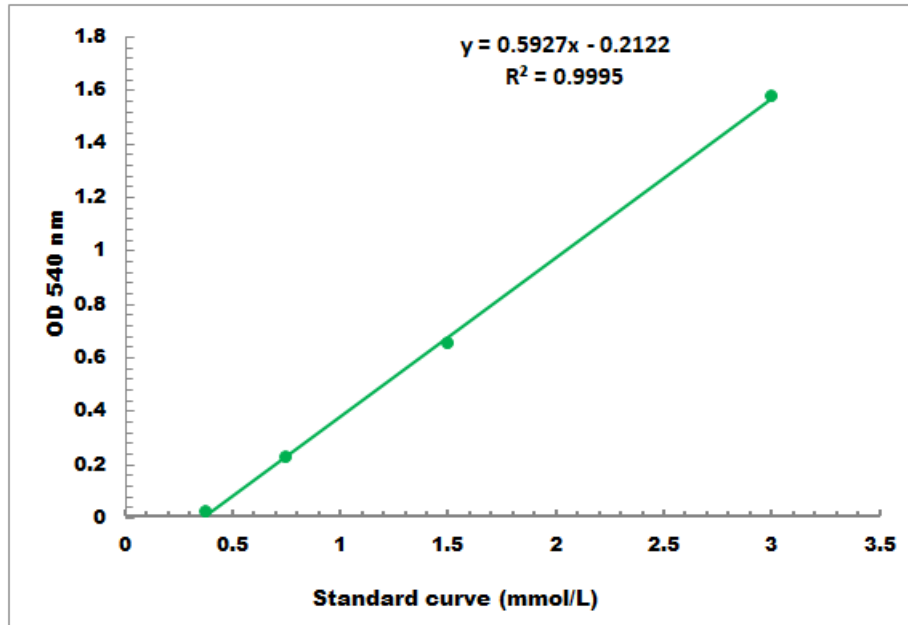

Detection Range: 0.3 mmol/L - 3 mmol/L